KERN & Sohn GmbH
Ziegelei 1
D-72336 Balingen
email: info@kern-sohn.com
Phone: +49-[0]7433- 9933-0
Fax: +49-[0]7433-9933-149
Internet: www.kern-sohn.com

Operating Manual(EN)

Laboratórna váha KERN PLE-N(SK)

Version 2.2
02/2012
GB





PLE-N-BA-e-1222

GB

KERN PLE-N

Version 2.2 02/2012

Operating Manual

Precision balances

English

Table of Contents

1 Technical Data 4

2 Declaration of conformity 5

3 Basic Information (General) 6

3.1 Proper use 6

3.2 Improper Use 6

3.3 Warranty 6

3.4 Monitoring of Test Resources 6

4 Basic Safety Precautions 7

4.1 Pay attention to the instructions in the Operation Manual 7

4.2 Personnel training 7

5 Transportation & Storage 7

5.1 Testing upon acceptance 7

5.2 Packaging / return transport 7

6 Unpacking, Setup and Commissioning 8

6.1 Installation Site, Location of Use 8

6.2 Unpacking 8

6.2.1 Placing 8

6.2.2 Scope of delivery / serial accessories 8

6.3 Appliance overview 9

6.4 Controls 10

6.4.1 Overview of display 10

6.4.2 Keyboard overview 10

6.5 Connect and switch-on power supply 11

6.6 Rechargeable battery operation 11

6.7 Connection of peripheral devices 12

6.8 Initial Commissioning 12

6.8.1 Stability display 12

6.8.2 Balance zero display 12

7 Adjustment 12

7.1.1 Adjustment with recommended adjustment weight (factory setting) 13

7.1.2 Adjustment with weights of other nominal values 14

8 Basic Operation 15
9 User menu 16
9.1 Weighing unit 19
9.2 Data output type 20
9.3 Baud rate 21
9.4 Auto Zero 22
9.5 Filter 24
9.6 Standstill control display 25
9.7 Display background illumination 26
9.8 Automatic switch-off function „AUTO OFF“ in stand-by mode 27
10 User menu 28
10.1 Parts counting 29
10.1.1 Switching over between quantity and weight display 31
10.1.2 Automatic reference optimization 31
10.1.3 Numeric entering of the reference weight 32
10.2 Density determination (Hydrostatic weighing) 33
10.2.1 Density determination of solids 33
10.2.2 Determining density of liquids 35
10.3 Checkweighing 37
10.4 Percent determination 39
10.4.1 Entering the reference weight by weighing 39
10.4.2 Numeric entering of the reference weight 40
10.5 Peak value function 41
11 Data output RS 232C 42
11.1 Technical Data 42
11.2 Pin allocation of balance output plug 42
11.3 Interface 43
11.4 Data transfer 43
11.5 Format for data transmission 44
11.6 Remote control instructions 45
11.7 Printer mode 45
12 Error messages 47
13 Service, maintenance, disposal 47
13.1 Cleaning 47
13.2 Service, maintenance 47
13.3 Disposal 47
14 Instant help 48

English

1 Technical Data

KERN	PLE 420-3N	PLE 4200-2N
Weighing range (max)	420 g	4200 g
Readability (d)	0.001 g	0.01 g
Reproducibility	0.002 g	0.02 g
Linearity	± 0.004 g	± 0.04 g
Stabilization time (typical)	2 sec	2 sec
Minimum unit weight at piece counting	0.005 g	0.05 g
Warm-up time	4 hours	
Recommended adjustment weight, not added (class)	400 g (E2)	4000 g (E2)
Reference quantities at piece counting	10, 25, 50, 100	
Weighing Units	ct, dwt, g, gn, mg, mo, oz, ozt, t	
Electric Supply	220V-240V, AC 50Hz	
Operating temperature	+ 10° C …. + 30° C	
Humidity of air	max. 80 % (not condensing)	
Housing (B x D x H) mm	185 x 250 x 80	
Dimensions of windshield (B x D x H) mm	150 (inside) 160 (outside)	
Weighing plate (stainless steel)	Ø 80	Ø 135
Weight kg (net)	2,5 kg	
Interface	RS 232C	

English

2 Declaration of conformity

KERN & Sohn GmbH
D-72322 Balingen-Frommern
Postbox 4052
email: info@kern-sohn.de
Phone: 0049-[0]7433- 9933-0
Fax: 0049-[0]7433-9933-149
Internet: www.kern-sohn.de

Declaration of conformity

EC-Konformitätserklärung
EC- Déclaration de conformité
EC-Dichiarazione di conformità
EC- Declaração de conformidade
EC-Deklaracja zgodności

EC-Declaration of -Conformity
EC-Declaración de Conformidad
EC-Conformiteitverklaring
EC- Prohlášení o shode
EC-Заявление о соответствии

D	Konformitäts-erklärung	Wir erklären hiermit, dass das Produkt, auf das sich diese Erklärung bezieht, mit den nachstehenden Normen übereinstimmt.
GB	Declaration of conformity	We hereby declare that the product to which this declaration refers conforms to the following standards.
CZ	Prohlášení o shode	Tímto prohlašujeme, že výrobek, kterého se toto prohlášení týká, je v souladu s níže uvedenými normami.
E	Declaración de conformidad	Manifestamos en la presente que el producto al que se refiere esta declaración está de acuerdo con las normas siguientes
F	Déclaration de conformité	Nous déclarons avec cela responsabilité que le produit, auquel se rapporte la présente déclaration, est conforme aux normes citées ci-après.
I	Dichiarazione di conformitá	Dichiariamo con ciò che il prodotto al quale la presente dichiarazione si riferisce è conforme alle norme di seguito citate.
NL	Conformiteit-verklaring	Wij verklaren hiermede dat het product, waarop deze verklaring betrekking heeft, met de hierna vermelde normen overeenstemt.
P	Declaração de conformidade	Declaramos por meio da presente que o produto no qual se refere esta declaração, corresponde às normas seguintes.
PL	Deklaracja zgodności	Niniejszym oświadczamy, że produkt, którego niniejsze oświadczenie dotyczy, jest zgodny z poniższymi normami.
RUS	Заявление о соответствии	Мы заявляем, что продукт, к которому относится данная декларация, соответствует перечисленным ниже нормам.

Electronic Balance: PLE-N

Mark applied	EU Directive	Standards
CE	2004/108/EC	EN 61326-1 (2006) EN 61000-3-2 (2006) EN 61000-3-3 (1995) + A1 (2001) + A2 (2005)
	2006/95/EC	EN 61010-1 (2001)

Date: 01.02.2011

Signature:

KERN & Sohn GmbH
Management

English

3 Basic Information (General)

3.1 Proper use

The balance you purchased is intended to determine the weighing value of material to be weighed. It is intended to be used as a “non-automatic“ balance, i.e. the material to be weighed is manually and carefully placed in the centre of the weighing plate. As soon as a stable weighing value is reached the weighing value can be read.

3.2 Improper Use

Do not use balance for dynamic weighing. In the event that small quantities are removed or added to the material to be weighed, incorrect weighing results can be displayed due to the “stability compensation“ in the balance. (Example: Slowly draining fluids from a container on the balance.)
Do not leave permanent load on the weighing plate. This may damage the measuring system.
Impacts and overloading exceeding the stated maximum load (max) of the balance, minus a possibly existing tare load, must be strictly avoided. Balance may be damage by this.
Never operate balance in explosive environment. The serial version is not explosion protected.
The structure of the balance may not be modified. This may lead to incorrect weighing results, safety-related faults and destruction of the balance.
The balance may only be used according to the described conditions. Other areas of use must be released by KERN in writing.

3.3 Warranty

Warranty claims shall be voided in case

- Our conditions in the operation manual are ignored
- The appliance is used outside the described uses
- The appliance is modified or opened
- Mechanical damage or damage by media, liquids, natural wear and tear
- The appliance is improperly set up or incorrectly electrically connected
- The measuring system is overloaded

3.4 Monitoring of Test Resources

In the framework of quality assurance the measuring-related properties of the balance and, if applicable, the testing weight, must be checked regularly. The responsible user must define a suitable interval as well as type and scope of this test. Information is available on KERN’s home page (www.kern-sohn.com with regard to the monitoring of balance test substances and the test weights required for this. In KERN’s accredited DKD calibration laboratory test weights and balances may be calibrated (return to the national standard) fast and at moderate cost.

4 Basic Safety Precautions

4.1 Pay attention to the instructions in the Operation Manual



Carefully read this operation manual before setup and commissioning, even if you are already familiar with KERN balances.

4.2 Personnel training

The appliance may only be operated and maintained by trained personnel.

5 Transportation & Storage

5.1 Testing upon acceptance

When receiving the appliance, please check packaging immediately, and the appliance itself when unpacking for possible visible damage.

5.2 Packaging / return transport



- ⇨ Keep all parts of the original packaging for a possibly required return.
- ⇨ Only use original packaging for returning.
- ⇨ Prior to dispatch disconnect all cables and remove loose/mobile parts.
- ⇨ Reattach possibly supplied transport securing devices.
- ⇨ Secure all parts such as the glass wind screen, the weighing platform, power unit etc. against shifting and damage.

6 Unpacking, Setup and Commissioning

6.1 Installation Site, Location of Use

The balances are designed in a way that reliable weighing results are achieved in common conditions of use.
You will work accurately and fast, if you select the right location for your balance.
Therefore, observe the following for the installation site:


- Place the balance on a firm, level surface;
- Avoid extreme heat as well as temperature fluctuation caused by installing next to a radiator or in the direct sunlight;
- Protect the balance against direct draughts due to open windows and doors;
- Avoid jarring during weighing;
- Protect the balance against high humidity, vapors and dust;
- Do not expose the device to extreme dampness for longer periods of time. Non-permitted condensation (condensation of air humidity on the appliance) may occur if a cold appliance is taken to a considerably warmer environment. In this case, acclimatize the disconnected appliance for ca. 2 hours at room temperature.
- Avoid static charge of goods to be weighed or weighing container.

Major display deviations (incorrect weighing results) may be experienced should electromagnetic fields (e.g. due to mobile phones or radio equipment), static electricity accumulations or instable power supply occur. Change location or remove source of interference.

6.2 Unpacking

Carefully remove the balance from the packaging, remove plastic cover and setup balance at the intended workstation.

6.2.1 Placing




Level balance with foot screws until the air bubble of the water balance is in the prescribed circle.

6.2.2 Scope of delivery / serial accessories

- Balance, Weighing plate
- Mains power supply
- Windshield
- Operating Manual

6.3 Appliance overview

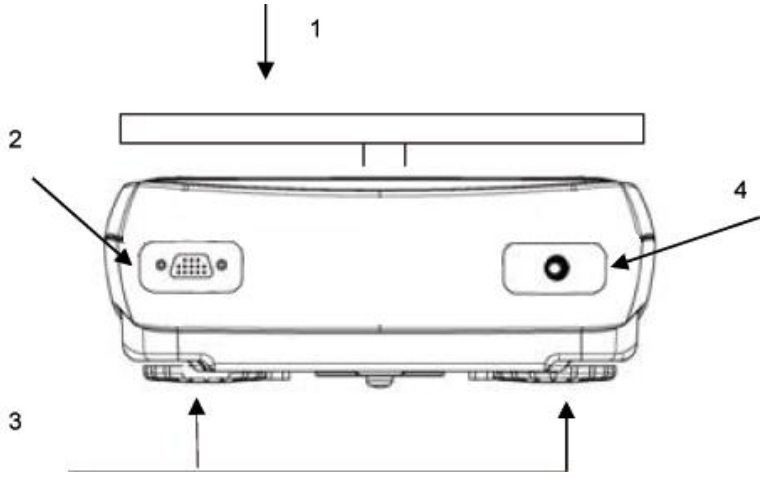


1. Weighing plate
2. RS232C interface
3. Foot screws
4. Mains adapter connection

English

6.4 Controls

6.4.1 Overview of display

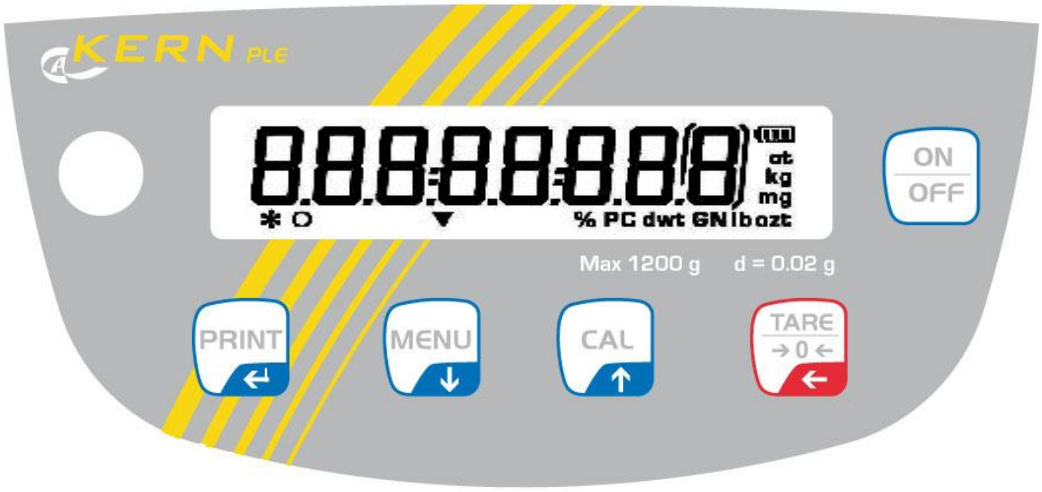

6.4.2 Keyboard overview

Key	Designation	Short key pressing	longtime pressed button until the acoustic signal gets mute
MENU	**MENU** button/	• Call-up application menu • Select menu items – scroll forward	• Call-up user menu • Exit user menu • Switch-over display
	Arrow button ↓	• numerical input – scroll backward	
ON OFF	**ON/OFF** switch	• Turn on/off • Exit user menu	
CAL	**CAL** button/	• Adjustment • Select menu items – scroll backward	
	Arrow button ↑	• Numerical input – scroll forward	
PRINT	**PRINT** button	• Calculate weighing data via interface • Confirm / store settings	
	Arrow button ←	• Numerical input – cipher selection	
TARE →0←	**TARE** button	• Taring • Zeroing	

6.5 Connect and switch-on power supply

Before connecting the mains adapter check if the printed voltage value is the same as the local supply voltage. Only use KERN original mains adapter. Using other makes requires consent by KERN.

⇨ Plug-in mains adapter in mains adapter bushing of the balance and connect to the mains.
⇨ The balance will carry out a self-test Then the balance is set into stand-by mode.



⇨ Press the **ON/OFF** key. When the zero display appears, the balance is ready for operation. When weighing with internal adjustment weight, adjustment first occurs automatically. During this process, „CAL“ will appear on the display.
⇨ Press the **ON/OFF** key anew. The balance is now in stand-by mode

For verified balances a warming-up time of 30 minutes must be observed.
After connecting the mains adapter a countdown starts.

6.6 Rechargeable battery operation (option)

The rechargeable battery is charged via the delivered power supply.
The operating time of the rechargeable battery is about 30h; charging time until complete recharging ca. 10h.
In the menu you can activate the AUTO-OFF function [time off], see chp. 9.8. According to menu settings, the balance switches automatically off in order to spare the battery.

When the balance is in battery mode the following symbols appear on the display:

	Battery charge sufficient
	Battery very low. Connect mains adapter as soon as possible to load the rechargeable battery.
	Voltage has dropped below prescribed minimum. Connect mains adapter to load the rechargeable battery.

English

6.7 Connection of peripheral devices

Before connecting or disconnecting of additional devices (printer, PC) to the data interface, always disconnect the balance from the power supply.
With your balance, only use accessories and peripheral devices by KERN, as they are ideally tuned to your balance.

6.8 Initial Commissioning

In order to obtain exact results with the electronic balances, your balance must have reached the operating temperature (see warming up time chap. 1).
During this warming up time the balance must be connected to the power supply (mains, accumulator or battery).
The accuracy of the balance depends on the local acceleration of gravity.
Strictly observe hints in chapter Adjustment.

6.8.1 Stability display

If the display shows the stability display [✱] the balance is in a stable status. If the status is instable the [✱] display disappears.

6.8.2 Balance zero display

If an exact zero reading is not displayed on the balance in spite of the weighing dish being empty, press the **TARE** button and the balance will start resetting to zero **[O]** .

7 Adjustment

As the acceleration value due to gravity is not the same at every location on earth, each balance must be coordinated - in compliance with the underlying physical weighing principle - to the existing acceleration due to gravity at its place of location (only if the balance has not already been adjusted to the location in the factory). This adjustment process must be carried out for the first commissioning, after each change of location as well as in case of fluctuating environment temperature. To receive accurate measuring values it is also recommended to adjust the balance periodically in weighing operation.

- ⇨ Observe stable environmental conditions. A warming up time (see chapter 1) is required for stabilization.
- ⇨ Ensure that there are no objects on the weighing plate.

7.1.1 Adjustment with recommended adjustment weight (factory setting)

Weight value of the required adjustment weight see chpt. 1 “Technical specifications“:



⇨ Ensure that there are no objects on the weighing plate. Press the **CAL** key



⇨ Wait until the weighed value for the required adjustment weight appears flashing.



⇨ **During** the flashing display put the required adjustment weight carefully in the center of the weighing plate.
The flashing display disappears.
After successful adjustment the balance automatically returns to weighing mode.

⇨ Take away adjustment weight



English

7.1.2 Adjustment with weights of other nominal values


Weights of different nominal values may be used for adjustment but are not optimal for technical measuring, possible adjustment points see table 1.
Info about adjustment weights can be found on the Internet at: http://www.kern-sohn.com



⇨ Ensure that there are no objects on the weighing plate. Press the **CAL** button and keep it pressed until the acoustic signal gets mute.



⇨ Wait until „load“ appears.

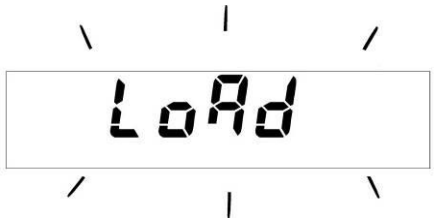

⇨ **During** the flashing display put the adjustment weight carefully in the center of the weighing plate.
The flashing display disappears.
After successful adjustment the balance automatically returns to weighing mode.

⇨ Take away adjustment weight




An error message will be displayed in the event of an adjustment error or incorrect adjustment weight. Wait until the balance is again in weighing mode and repeat the adjustment procedure.

8 Basic Operation

Start-up

In stand-by mode press ON/OFF button.
The balance is ready for weighing when the weight display appears.



Switching Off

Press ON/OFF button, the balance returns to the stand-by mode.

Simple weighing

⇨ Place goods to be weighed on balance


⇨ Wait until the stability display appears [✱]



⇨ Read weighing result.

Taring

⇨ Place the weighing box and press the **TARE** button.
„0-t“ is displayed.



⇨ After standstill control the zero display appears.



The weight of the container is now internally saved.

⇨ Weigh the material, the net weight will be indicated.

The weight of the weighing container will be displayed as a minus number after removing the weighing container.

The tare weight is saved until it is deleted. Remove the load from the balance and press the **TARE** button. „0-t“ is displayed, wait until the zero display appears.

The tare procedure can be repeated as many times as necessary, for example with initial weighing of several components for a mix (add-on weighing). The limit is reached when the total weighing range capacity is full.

English

9 User menu

The settings of the balance can be changed in the user menu. This way, the balance can be adjusted to individual weighing requirements.
By the factory the user menu has been set in a way that normally no more changes must be made, only at special conditions of use.

Navigation in the menu

Access to menu

In weighing mode press the **MENU** button and keep it pressed until the acoustic signal gets mute. The first menu item „units“ is displayed.

How to select menu items

Using the **MENU** button the individual menu items can be selected one after the other.

- ⇨ Scroll forward using **MENU** button
- ⇨ Scroll backward using **CAL** button

Change settings

Acknowledge selected menu item using **PRINT** button, the current setting is displayed. Each time the arrow buttons 🡻 🡹 are pressed the next setting will be displayed.

- ⇨ Scroll forward using **MENU** button
- ⇨ Scroll backward using **CAL** button

Save settings

Take over selection using the **PRINT** button.
Weighing balance returns to menu. Either make more settings in the menu or go back to menu mode as follows.

Exit menu/ back to weighing mode

Press the **MENU** button and keep it pressed until the acoustic signal gets mute. The balance returns automatically into weighing mode.

Menu overview

Menu item	Display	Selection	Description
Weighing unit (see chap. 9.1)	**Units**	**Gram**	Gramm
		Carat	Carat
		Ounce	Unze
		Pound	Pound
		PEnn	Pennyweight
		OuncEtr	Troy Unze
		GrAin	Grain
		tAEL Hon	Tael Hongkong
		tAEL SGP	Tael Singapore
		tAEL roc	Tael R.O.C.
		Momme	Momme
Data output type (see chap. 9.2)	**PC-Prtr**	**PC cont**	Continuous output
		PC CMd	Manual issue after pressing the **PRINT** button
		Print	not documented
Baudrate (see chap. 9.3)	**baud rt**	**br 1200**	
		br 2400	
		br 4800	
		br 9600	
Auto zero (see chap. 9.4)	**Auto 0**	**Au0 OFF**	Auto Zero switched off
		Au0 1	Auto Zero range ± ½ digit
		Au0 2	Auto Zero range ± 3 digits
		Au0 3	Auto Zero range ± 7 digits
		Au0 3E	Auto Zero range ± 7 digits in the whole weighing range
Filter (see chap. 9.5)	**Filter**	**Filt 1**	Setting for dispensing
		Filt 2	Sensitive and fast, very quiet set-up location
		Filt 3	Robust but slow, busy set-up locatio
Standstill control display (see chap. 9.6)	**Stabil**	**Stab 1**	Standstill control fast – very quiet set-up location
		Stab 2	Standstill control fast + exact – quiet set-up location
		Stab 3	Standstill control exact – very set-up location

Backlight (see chap. 9.7)	**Blt**	**on**	Backlight on
		off	Backlight off
		Auto	Backlight automatically switched off 3 seconds after achieving stable weighing value. Changes in weight or pressing of keys will automatically result in backlight switching on again.
AUTO OFF in stand-by mode (see chap. 9.8)	**time off**	**disab**	AUTO-OFF off
		2 Min	AUTO-OFF after 2 minutes without changing the weight
		5 Min	AUTO-OFF after 5 minutes without changing the weight
		15 Min	AUTO-OFF after 15 minutes without changing the weight
Adjustment (see chap. 7)	**Calib**	**E-Cal**	Adjustment with external weight, locked for verifiable units
	End		

9.1 Weighing unit

According to requirements the balance can be switched-over into different units (in verified balances not all the units are available, see chap. 1 „Technical specifications). Selected weighing unit will be retained even after disconnection from the mains.

⇨ In weighing mode press the **MENU** button and keep it pressed until the acoustic signal gets mute. The first menu item „units“ is displayed.




⇨ Acknowledge using **PRINT** button, the current setting is displayed.



⇨ Press the arrow keys 🡻 🡹 to select desired setting.

Scroll forward using **MENU** button

Scroll backward using **CAL** button

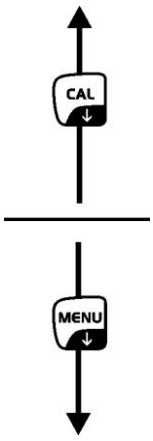

Symbol	Weighing unit	Conversion factor 1g =
Gram	GRAMS	1.
Carat	CARATS	5.
Ounce	OUNCE	0.035273962
Pound	POUNDS	0.0022046226
PEnn	PENNYWEIGHTS	0.643014931
OuncEtr	OUNCE TROY	0.032150747
GrAin	GRAIN	15.43235835
tAEL Hon	HONG KONG TAEL	0.02671725
tAEL SGP	SYNGAPORE TAEL	0.02646063
tAEL roc	R.O.C. TAEL	0.02666666
Momme	MOMME	0.2667

⇨ Take over selection using the **PRINT** button.
Weighing balance returns to menu. Either make more settings in the menu or go back to weighing mode as follows.

⇨ Press the **MENU** button and keep it pressed until the acoustic signal gets mute. The balance returns automatically into weighing mode.

9.2 Data output type

⇨ In weighing mode press the **MENU** button and keep it pressed until the acoustic signal gets mute.



⇨ Press **MENU** button




⇨ Acknowledge using **PRINT** button, the current setting is displayed.

⇨ Press the arrow keys 🡻 🡹 to select desired setting.

Scroll forward using **MENU** button

Scroll backward using **CAL** button

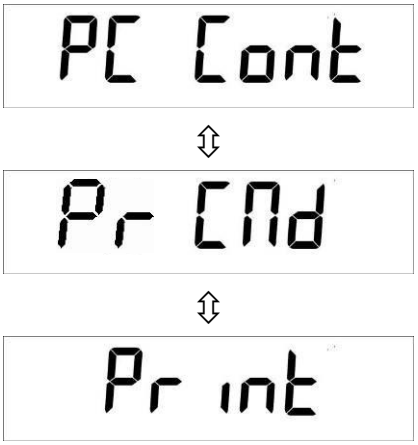

„PC cont“ = Continuous output

„PC CMd“ = Manual issue after pressing the **PRINT** button

„Print“ = not documented

⇨ Take over selection using the **PRINT** button.
Weighing balance returns to menu. Either make more settings in the menu or go back to weighing mode as follows.

⇨ Press the **MENU** button and keep it pressed until the acoustic signal gets mute.
The balance returns automatically into weighing mode.



9.3 Baud rate

⇨ In weighing mode press the **MENU** button and keep it pressed until the acoustic signal gets mute.



⇨ Press **MENU** button repeatedly




⇨ Acknowledge using **PRINT** button, the current setting is displayed.

⇨ Press the arrow keys ↓ ↑ to select desired setting.

Scroll forward using **MENU** button

Scroll backward using **CAL** button

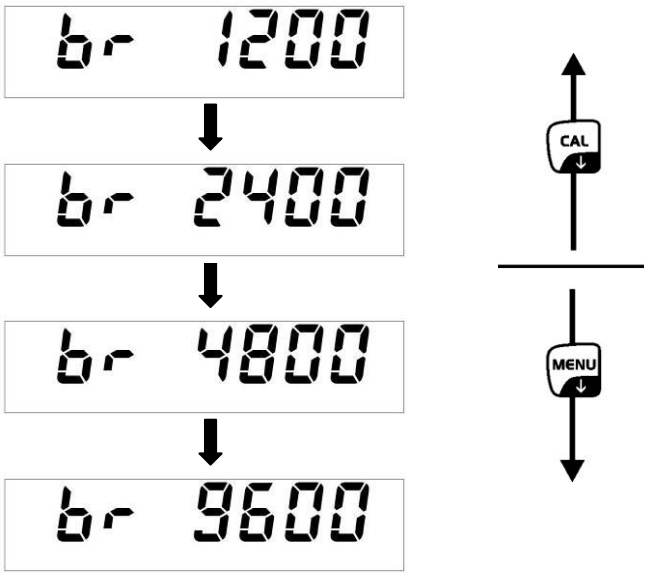

⇨ Take over selection using the **PRINT** button.
Weighing balance returns to menu. Either make more settings in the menu or go back to weighing mode as follows.

⇨ Press the **MENU** button and keep it pressed until the acoustic signal gets mute.
The balance returns automatically into weighing mode.



English

9.4 Auto Zero

Under this menu item the automatic zero point correction can be switched on or off. In switched-on-state the zero point is automatically corrected at drift or when dirty.

Information:
In the event that small quantities are removed or added to the material to be weighed, incorrect weighing results can be displayed due to the “stability compensation“ in the balance. (e.g. slow flow of liquids from a container placed on the balance, evaporating processes).
When apportioning involves small variations of weight, it is advisable to switch off this function.

⇨ In weighing mode press the **MENU** button and keep it pressed until the acoustic signal gets mute.



⇨ Press **MENU** button repeatedly




⇨ Acknowledge using **PRINT** button, the current setting is displayed.

⇨ Press the arrow keys 🡻 🡹 to select desired setting.

Scroll forward using **MENU** button

Scroll backward using **CAL** button

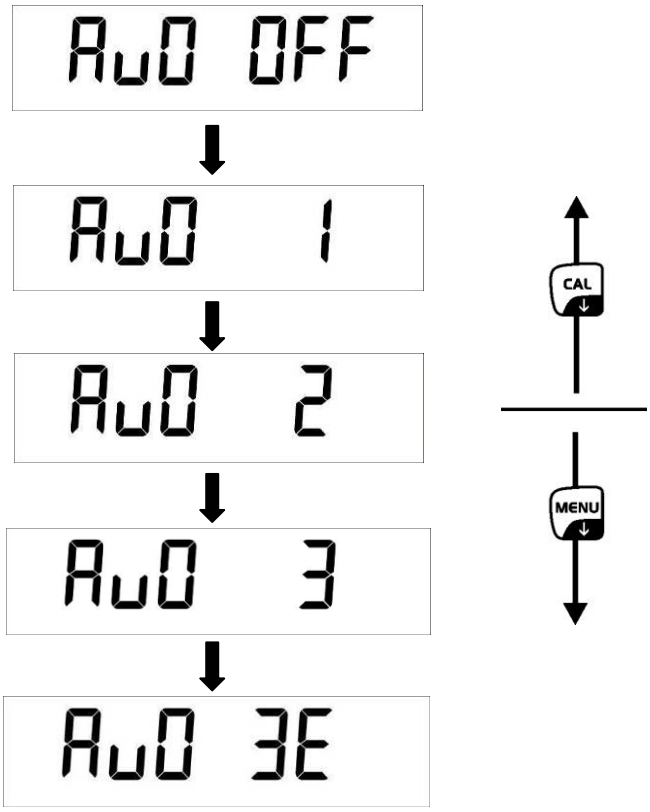

Au0 OFF = Auto Zero switched off
Au0 1 = Auto Zero range ± ½ digit
Au0 2 = Auto Zero range ± 3 digits
Au0 3 = Auto Zero range ± 7 digits
Au0 3E = Auto Zero range ± 7 digits in the whole weighing range

⇨ Take over selection using the **PRINT** button.
Weighing balance returns to menu. Either make more settings in the menu or go back to weighing mode as follows.

⇨ Press the **MENU** button and keep it pressed until the acoustic signal gets mute.
The balance returns automatically into weighing mode.



English

9.5 Filter

This menu item allows the balance to be set according to specific ambient conditions and measuring purposes.

⇨ In weighing mode press the **MENU** button and keep it pressed until the acoustic signal gets mute.



⇨ Press **MENU** button repeatedly




⇨ Acknowledge using **PRINT** button, the current setting is displayed.

⇨ Press the arrow keys 🡻 🡹 to select desired setting.

Scroll forward using **MENU** button

Scroll backward using **CAL** button

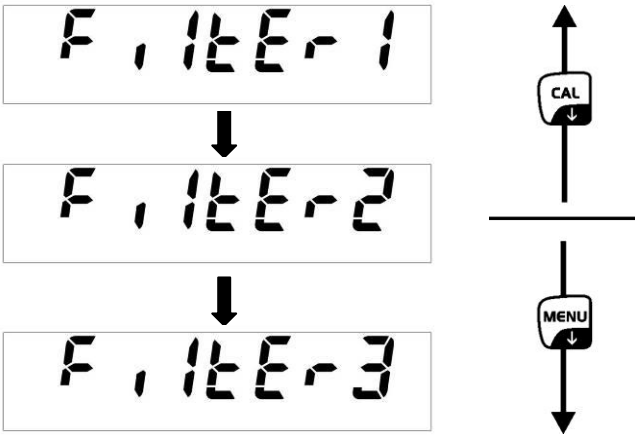

FILTER 1: Setting for dispensing
FILTER 2: Sensitive and fast, very quiet set-up location.
FILTER 3: Robust but slow, busy set-up location.

⇨ Take over selection using the **PRINT** button.
Weighing balance returns to menu. Either make more settings in the menu or go back to weighing mode as follows.

⇨ Press the **MENU** button and keep it pressed until the acoustic signal gets mute.
The balance returns automatically into weighing mode.



9.6 Standstill control display

⇨ In weighing mode press the **MENU** button and keep it pressed until the acoustic signal gets mute.



⇨ Press **MENU** button repeatedly




⇨ Acknowledge using **PRINT** button, the current setting is displayed.

⇨ Press the arrow keys 🡻 🡹 to select desired setting.

Scroll forward using **MENU** button

Scroll backward using **CAL** button

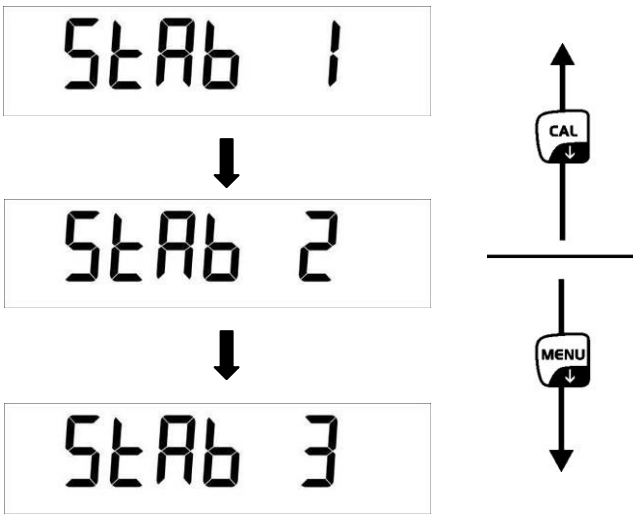

STAB 1: Standstill control fast – very quiet set-up location
STAB 2: Standstill control fast + exact – quiet set-up location
STAB 3: Standstill control exact – very set-up location.

⇨ Take over selection using the **PRINT** button.
Weighing balance returns to menu. Either make more settings in the menu or go back to weighing mode as follows.

⇨ Press the **MENU** button and keep it pressed until the acoustic signal gets mute.
The balance returns automatically into weighing mode.



English

9.7 Display background illumination

⇨ In weighing mode press the **MENU** button and keep it pressed until the acoustic signal gets mute.



⇨ Press **MENU** button repeatedly




⇨ Acknowledge using **PRINT** button, the current setting is displayed.

⇨ Press the arrow keys ↓ ↑ to select desired setting.

Scroll forward using **MENU** button

Scroll backward using **CAL** button

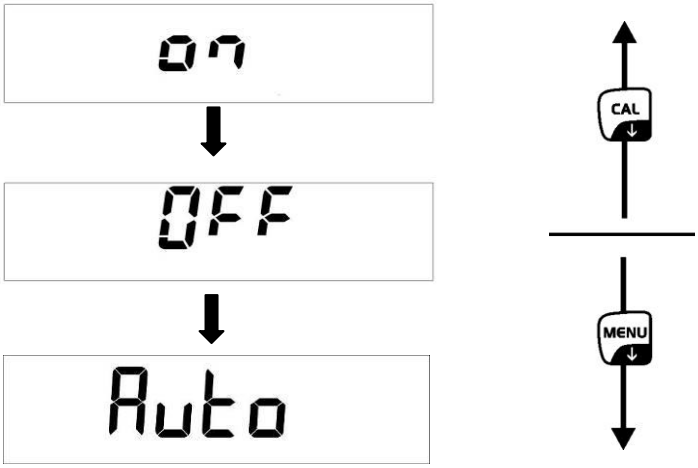

ON Background illumination on

OFF Background illumination off

Auto Backlighting automatically switched off 3 seconds after achieving stable weighing value. Changes in weight or pressing of keys will automatically result in backlight switching on again.

⇨ Take over selection using the **PRINT** button.
Weighing balance returns to menu. Either make more settings in the menu or go back to weighing mode as follows.

⇨ Press the **MENU** button and keep it pressed until the acoustic signal gets mute.
The balance returns automatically into weighing mode.



9.8 Automatic switch-off function „AUTO OFF“ in stand-by mode

⇨ In weighing mode press the **MENU** button and keep it pressed until the acoustic signal gets mute.



⇨ Press **MENU** button repeatedly




⇨ Acknowledge using **PRINT** button, the current setting is displayed.

⇨ Press the arrow keys 🡻 🡹 to select desired setting.

Scroll forward using **MENU** button

Scroll backward using **CAL** button

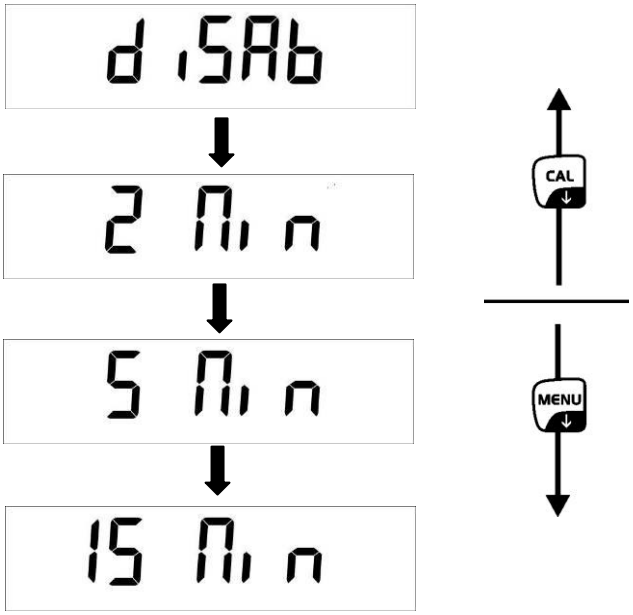

disab = AUTO-OFF switched off
2 Min = AUTO-OFF after 2 minutes without changing the weight
5 Min = AUTO-OFF after 5 minutes without changing the weight
15 Min = AUTO-OFF after 15 minutes without changing the weight

⇨ Take over selection using the **PRINT** button.
Weighing balance returns to menu. Either make more settings in the menu or go back to weighing mode as follows.

⇨ Press the **MENU** button and keep it pressed until the acoustic signal gets mute.
The balance returns automatically into weighing mode.



English

10 User menu

The following operating modes may be enabled/disabled in the user menu:

Count	Parts counting
⇩	
Dens	Density determination of solids/liquids
⇩	
HoL	Checkweighing
⇩	
Perc	Percent determination
⇩	
M Load	Peak value function
⇩	
End	

Navigation in the menu

Access to menu

In weighing mode press **MENU** button. The first menu item „count“ is displayed.

How to select menu items

Using the **MENU** button the individual menu items can be selected one after the other.

⇨ Scroll forward using **MENU** button

⇨ Scroll backward using **CAL** button

Change settings

Acknowledge selected menu item using **PRINT** button, the current setting is displayed. Each time the arrow buttons 🡻 🡹 are pressed the next setting will be displayed.

⇨ Scroll forward using **MENU** button

⇨ Scroll backward using **CAL** button

Save settings

Take over selection using the **PRINT** button.
Weighing balance returns to menu. Either make more settings in the menu or go back to menu mode as follows.


Exit menu/ back to weighing mode

Press the **MENU** button and keep it pressed until the acoustic signal gets mute. The balance returns automatically into weighing mode.

10.1 Parts counting

Before the balance can count parts, it must know the average part weight (i.e. reference). Proceed by putting on a certain number of the parts to be counted. The balance determines the total weight and divides it by the number of parts, the so-called reference quantity. Counting is then carried out on the basis of the calculated average piece weight.
As a rule:
The higher the reference quantity the higher the counting exactness.

⇨ In weighing mode press **MENU** button. The first menu item „count“ is displayed.



⇨ Acknowledge using **PRINT** button, the current reference quantity is displayed.




⇨ Using the arrow buttons ↓ ↑ select reference quantity (10, 25, 50, 100 or manual = numerical input of the reference weight, see chap. 10.1.3).

Scroll forward using **MENU** button

Scroll backward using **CAL** button

⇨ If using a weighing container, put this before pressing the **PRINT** button. The taring process is automatically started. „0-t“ is displayed.



⇨ Confirm selected reference number of items by pressing the **PRINT** button.



⇨ Place as many pieces to add-up as required by the set reference piece number.

⇨ Acknowledge using **PRINT** button and wait for standstill control.
After successful reference determination the current quantity is displayed.



⇨ Remove reference weight. The balance is now in parts counting mode counting all units on the weighing plate.

English

If it was impossible to determine a reference due to instable goods to be weighed or an insufficient reference weight, the following display will appear during reference calculation.

- **ERR04** = smallest counting weight not achieved
- **Add SMP**=if the placed quantity for a correct reference determination is too small, more parts must be placed as follows.



⇨ Place more parts, but at least the double quantity.

⇨ Press the **PRINT** button, the reference weight is calculated anew.



The placed quantity is always too small, add more parts and acknowledge using the **PRINT** button. Repeat the procedure until the piece counter display appears.



Placed quantity sufficient for reference determination. Remove reference weight. The balance is now in parts counting mode counting all units on the weighing plate.


Return to weighing mode

⇨ Press the **ON/OFF** key.



10.1.1 Switching over between quantity and weight display

⇨ Place load on pan and read the number of pieces.

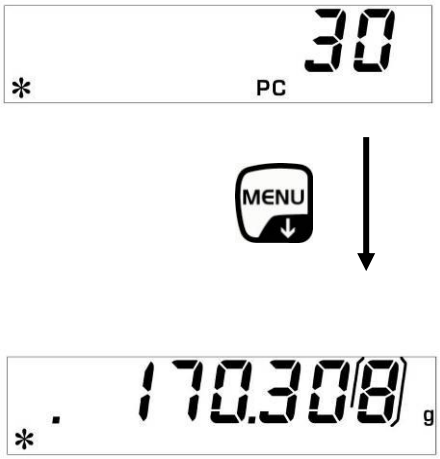

⇨ Press **MENU** button, the total weight of the placed parts is displayed.

or

⇨ Press the **MENU** button and keep it pressed until the acoustic signal gets mute, the average weight of a single piece is displayed.

⇨ Back to quantity display press **MENU** button again.

10.1.2 Automatic reference optimization

In order to improve the counting exactness, the reference can be optimised by adding more pieces. At every reference optimisation, the reference weight is calculated anew. As the additional pieces increase the base for the calculation, the reference also becomes more exact.

⇨ Leave the piece number on the weighing plate after setting the reference weight

⇨ Duplicate the number of pieces on the weighing plate and wait until the acoustic signal sounds. The reference weight is calculated anew.

⇨ Either repeat the reference optimisation by adding more pieces (max. 255 pieces) or start the counting process.


The automatic reference optimisation is not active when the reference weight is entered numerically.

English

10.1.3 Numeric entering of the reference weight

If you know the reference weight/piece you can enter this via the numeric keyboard.

⇨ In weighing mode press **MENU** button. The first menu item „count“ is displayed.



⇨ Acknowledge using **PRINT** button, the current reference quantity is displayed.



⇨ Press the arrow buttons ↓ ↑ to select the parameters manually.



⇨ Press the arrow buttons ↓ ↑ ← to enter the known reference weight.

⇨ If using a weighing container, put this before pressing the **PRINT** button.
The taring process is automatically started. „0-t“ is displayed.



⇨ Place load on pan and read the number of pieces.



⇨ Press **MENU** button, the total weight of the placed parts is displayed.



⇨ Back to quantity display press **MENU** button again.

Return to weighing mode

⇨ Press the **ON/OFF** key



10.2 Density determination (Hydrostatic weighing)


Density is the relationship of weight [g] : volume [cm^3]. The weight is determined by weighing the sample in air. The volume results from the ascending force [g] of the sample dipped in a liquid. The density [g/cm^3] of that liquid is known (principle of Archimedes).
The density is determined with help of the underfloor weighing device.

10.2.1 Density determination of solids

Prepare the balance as follows:

- Switch off the balance
- Remove the weighing pan and carefully turn over the weighing balance.
- Screw-in hook for underfloor weighing (option)
- Place weighing balance over an opening
- Hook-in the sample support
- Fill measuring liquid in a vessel e.g. beaker) and temper it.

⇨ In weighing mode press **MENU** button. The first menu item „count“ is displayed.




⇨ Press **MENU** button



⇨ Acknowledge using **PRINT** button, the current setting is displayed.

⇨ Using **MENU** button select **„d SoLid**“



⇨ Confirm by pressing the **PRINT** button.



⇨ Use the arrow buttons 🡻 🡹 🡸 to enter density of the measuring fluid.

⇨ Confirm input by pressing the **PRINT** button.

⇨ The display for weight determination of the "sample in air“ appears.



⇨ Confirm by pressing the **PRINT** button.

⇨ If necessary, tare and put the sample.

⇨ Wait until the weight display of the weighing balance has become stable and then press the **PRINT** button. „WEI AIR“ appears flashing.

⇨ The display for weight determination of the "sample in the measuring fluid“ appears.



⇨ Immerse sample holder and tare by pressing the **TARE**-key

⇨ Place sample and immerse it
Make sure that the sample holder does not touch the beaker.

⇨ Wait until the weight display of the weighing balance has become stable and then press the **PRINT** button. „WEI LIQ“ appears flashing.

⇨ The density of the sample is shown




Return to weighing mode

⇨ Press the **ON/OFF** key



⇨ or use the **MENU** button to start a new measuring cycle.

If at the density determination errors have appeared, „d-----„ is displayed.




10.2.2 Determining density of liquids

⇨ Fill sample liquid into a vessel, e.g. a pitcher.

⇨ Heat sample liquid until temperature is constant.

⇨ Prepare a glass sinker with known density

⇨ In weighing mode press **MENU** button. The first menu item „count“ is displayed.



⇨ Press **MENU** button



⇨ Acknowledge using **PRINT** button, the current setting is displayed.

⇨ Using **MENU** button select **„d Liquid**“



⇨ Confirm by pressing the **PRINT** button.



⇨ Use the arrow buttons 🡻 🡹 🡸 to enter density of the glass sinker.

⇨ Confirm input by pressing the **PRINT** button.

English

⇨ The display for weight determination of the "glass sinker in air“ appears.



⇨ Confirm by pressing the **PRINT** button.

⇨ Tare if necessary and hook on the glass sinker centrically.

⇨ Wait until the weight display of the weighing balance has become stable and then press the **PRINT** button. „WEI AIR“ appears flashing.

⇨ The display for weight determination of the "glass sinker in sample liquid“ appears.



⇨ Tare if necessary and immerse the sinker into the measuring fluid

⇨ Wait until the weight display of the weighing balance has become stable and then press the **PRINT** button. „WEI LIQ“ appears flashing.

⇨ The density of the sample fluid is shown




Return to weighing mode

⇨ Press the **ON/OFF** key



⇨ or use the **MENU** button to start a new measuring cycle.

If at the density determination errors have appeared, „d-----„ is displayed.




10.3 Checkweighing


An upper and a lower limit value can be established to ensure that the weighed goods are exactly within the established tolerance limits.
The display **[L]**, **[ok]** or **[H]** shows whether the goods to be weighed are within the two tolerance limits.



Goods to be weighed below tolerance limit

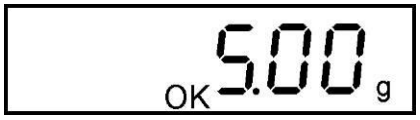


Goods to be weighed within tolerance range




Goods to be weighed above tolerance limit

The indetermination if the goods to be weighed are within the tolerance limits, can additionally be given by an acoustic signal.

⇨ In weighing mode press **MENU** button. The first menu item „count“ is displayed.



⇨ Press **MENU** button repeatedly

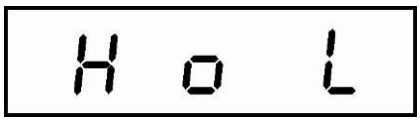

⇨ Confirm using the **PRINT** button, the display to enter the lower tolerance limit appears.



⇨ Enter the lower limit value using the arrow buttons ↓ ↑ ←

⇨ Confirm using the **PRINT** button, the display to enter the upper tolerance limit appears.



⇨ Enter the upper limit value using the arrow buttons ↓ ↑ ←

⇨ Confirm using the **PRINT** button, the display to adjust the signal tone appears.

⇨ Select the desired settings by pressing the **MENU** button

Beep off Signal tone switched off

Beep on Signal tone on, if weighed goods are within tolerance range

⇨ Confirm by pressing the **PRINT** button.
The balance is now in checkweighing mode.

⇨ Put on goods to be weighed, tolerance control is started

Return to weighing mode

⇨ Press the **ON/OFF** key



English

10.4 Percent determination

Percent determination allows weight display in percent, in relation to a reference weight.

10.4.1 Entering the reference weight by weighing

⇨ In weighing mode press **MENU** button. The first menu item „count“ is displayed.




⇨ Press **MENU** button repeatedly




⇨ Acknowledge using **PRINT** button, the current setting is displayed.

⇨ Using **MENU** button select **„PErc A**“

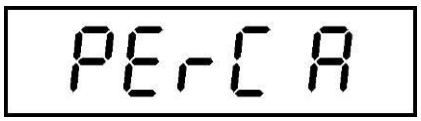


⇨ If using a weighing container, put this before pressing the **PRINT** button. The taring process is automatically started. „0-t“ is displayed.





⇨ Put on reference weight (=100 %)

⇨ Wait until the weight display of the balance has become stable and then press the **PRINT** button. The weight is adopted as reference (100%).

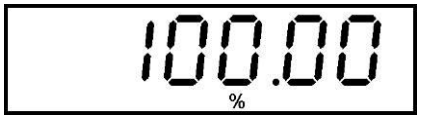


⇨ Remove reference weight. From now the balance is in percent determining mode.

⇨ Place goods to be weighed on balance.
The weight of the sample is displayed in percentage in terms of the reference weight.

10.4.2 Numeric entering of the reference weight

⇨ In weighing mode press **MENU** button. The first menu item „count“ is displayed.



⇨ Press **MENU** button repeatedly




⇨ Acknowledge using **PRINT** button, the current setting is displayed.

⇨ Using **MENU** button select **„PErc n**“




⇨ Confirm using the **PRINT** button, the display to enter the reference weight appears.



⇨ Press the arrow buttons 🡻 🡹 🡸 to enter the reference weight (100%).

⇨ Confirm input by pressing the **PRINT** button. From now the balance is in percent determining mode.



⇨ Place goods to be weighed on balance.
The weight of the sample is displayed in percentage in terms of the reference weight.

Return to weighing mode

⇨ Press the **ON/OFF** key



10.5 Peak value function

This function displays the highest load value (peak value) of a weighing.
The peak value remains in the display until it will be deleted.

⇨ In weighing mode press **MENU** button. The first menu item „count“ is displayed.



⇨ Press **MENU** button repeatedly



⇨ Confirm using **PRINT** button, the taring process is automatically started. „0-t“ is displayed.
From here the balance is in peak value mode, where a „M” pops up.



⇨ Load weighing plate. The maximum load value is displayed.



⇨ The peak value remains in the display until the **TARE** button is pressed. Then the balance is ready for further measurements.


Return to weighing mode

⇨ Press the **ON/OFF** key



English


11 Data output RS 232C

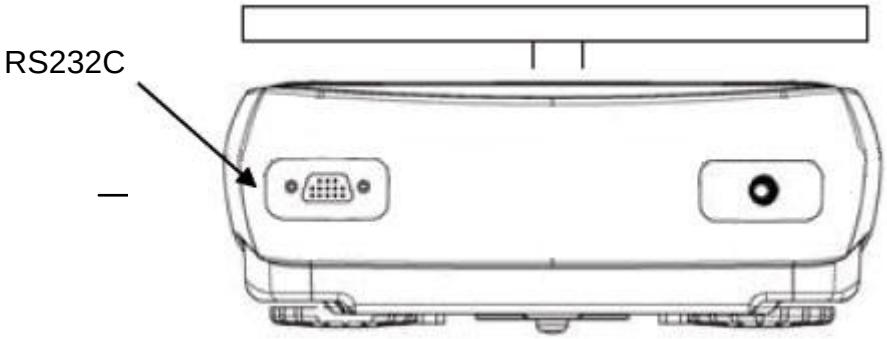

11.1 Technical Data

- 8-bit ASCII Code
- 8 data bits, 1 stop bit, no parity bit
- Baud rate optional from 1200 - 9600 Baud
- For operation with interface faultless operation is only ensured with the correct KERN – interface cable (max. 2m)


11.2 Pin allocation of balance output plug

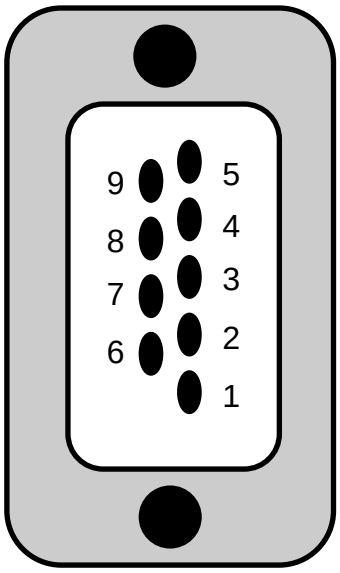


Pin 2:	Tx Signal
Pin 3:	Rx Signal
Pin 5:	Gnd

11.3 Interface


- Balance – PC 25-pole

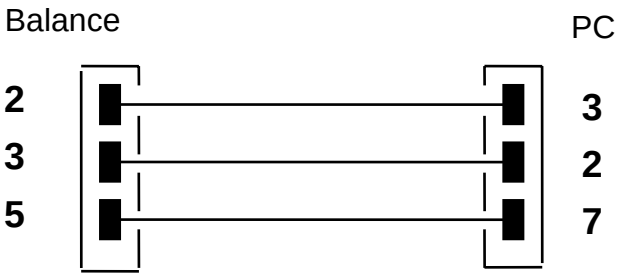

- Balance – PC 9-pole

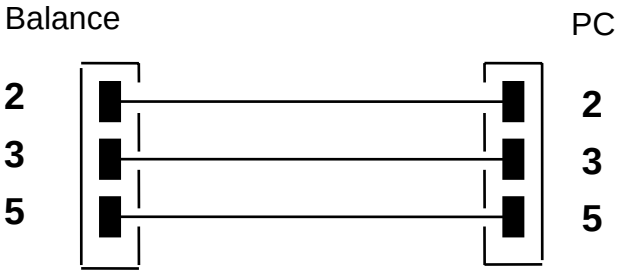

- Balance - printer

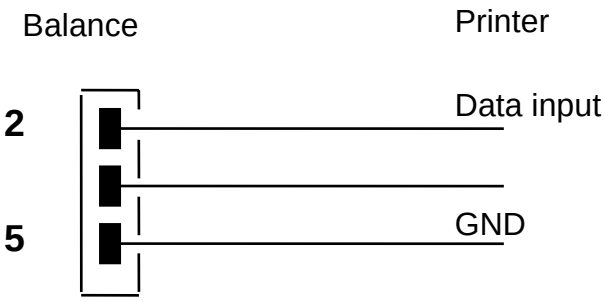

11.4 Data transfer

The data set consists of the following 14 characters:

1. Character	sign -/ blank (weighing value)
2-9. Character	weight or other data
10-12. Character	weighing unit
13. Character	stability display
14. Character	carriage return
15. Character	line feed

11.5 Format for data transmission

At stable weight the format is transferred after pressing the **PRINT** button.

Weighing mode (continuous output and remote control command)

1°	2°	3°	4°	5°	6°	7°	8°	9°	10°	11°	12°	13°	14°	15°r
Character	Weight								Weighing unit			Stability	CR	LF

Density determination (only remote control command)

1°	2°	3°	4°	5°	6°	7°	8°	9°	10°	11°	12°	13°	14°	15°	16°	17°
d	=	Density							Blank	Weighing unit					CR	LF

Counting (only remote control command)

Number of pieces

1°.	2°	3°	4°	5°	6°	7°	8°	9°	10°	11°	12°	13°	14°	15°	16°
Pcs			:	Blank				Quantity							

Weight of placed pieces

1°.	2°	3°	4°	5°	6°	7°	8°	9°	10°	11°	12°	13°	14°	15°	16°	17°	18°	19°	20°
Weight						:	space	Measuring Value								space	g	space	S

Average parts weight

1°.	2°	3°	4°	5°	6°	7°	8°	9°	10°	11°	12°	13°	14°	15°	16°	17°	18°
PMU average piece weight			:	Blank				Measuring Value								space	g

11.6 Remote control instructions

Instruction:	Function
“T” = H54	Taring
“C” = H43	Adjustment
“E” = H45	Enter
“M” = H4D	Menu
“O” = H4F	ON/OFF

11.7 Printer mode

The following conditions must be met to provide successful communication between the weighing balance and the printer.

- Use a suitable cable to connect the weighing balance to the interface of the printer. Faultless operation requires an adequate KERN interface cable.
- The Baud rates of balance and printer must agree, see chap. 9.3.

Printout examples:

Weighing mode/peak value function

```
…….          22.000 g
```

Density determination

```
d=   2.80066  g/cm3d
```

d Measuring value „Density“

Parts counting

```
Pcs              100
Weight:    300.000 g
PMU:         3.000 g
```

PCS Number of pieces

Weight Weight of placed pieces

PMU Average parts weight

Percent determination

```
Perc.             20 %
Weight:       30.000 g
```

Perc Display value in [%]

Weight Display value in [g]

12 Error messages

ERR01	Weight value instable or zeroing not possible. Check the environmental conditions.
ERR02	Adjustment error, e.g. environmental conditions instable
ERR03	Adjustment error e.g. incorrect adjustment weight}
ERR04	Piece weight too small/instable
ERR05	Data transfer not possible, as weighing value is instable. Check the environmental conditions.
ERR06	Weighing value in density determining mode instable. Check the environmental conditions.
"**UNLOAD**":	Weighing range not achieved. Check position of the weighing plate
"**CAL But**"	Adjust balance
	Weighing range exceeded, placed load exceeds the capacity of the balance. Unload the balance.
	Weighing range not reached, e.g. weighing plate not in place

13 Service, maintenance, disposal

13.1 Cleaning

Before cleaning, please disconnect the appliance from the operating voltage.

Please do not use aggressive cleaning agents (solvents or similar agents), but a cloth dampened with mild soap suds. Ensure that no liquid penetrates into the device and wipe with a dry soft cloth.
Loose residue sample/powder can be removed carefully with a brush or manual vacuum cleaner.

Spilled weighing goods must be removed immediately.

13.2 Service, maintenance

The appliance may only be opened by trained service technicians who are authorized by KERN.
Before opening, disconnect from power supply.

13.3 Disposal

Disposal of packaging and appliance must be carried out by operator according to valid national or regional law of the location where the appliance is used.

14 Instant help

In case of an error in the program process, briefly turn off the balance and disconnect from power supply. The weighing process must then be restarted from the beginning.

Help:

Fault	**Possible cause**
The displayed weight does not glow.	• The balance is not switched on. • The mains supply connection has been interrupted (mains cable not plugged in/faulty). • Power supply interrupted. • (Rechargeable) batteries are inserted incorrectly or empty • No (rechargeable) batteries inserted.
The displayed weight is permanently changing	• Draught/air movement • Table/floor vibrations • Weighing plate has contact with other objects. • Electromagnetic fields / static charging (choose different location/switch off interfering device if possible)
The weighing result is obviously incorrect	• The display of the balance is not at zero • Adjustment is no longer correct. • Great fluctuations in temperature. • Warm-up time was ignored. • Electromagnetic fields / static charging (choose different location/switch off interfering device if possible)

Should other error messages occur, switch balance off and then on again. If the error message remains inform manufacturer.